

FIG. 1

FIG. 2 is a cross-sectional view of the device in a closed position.

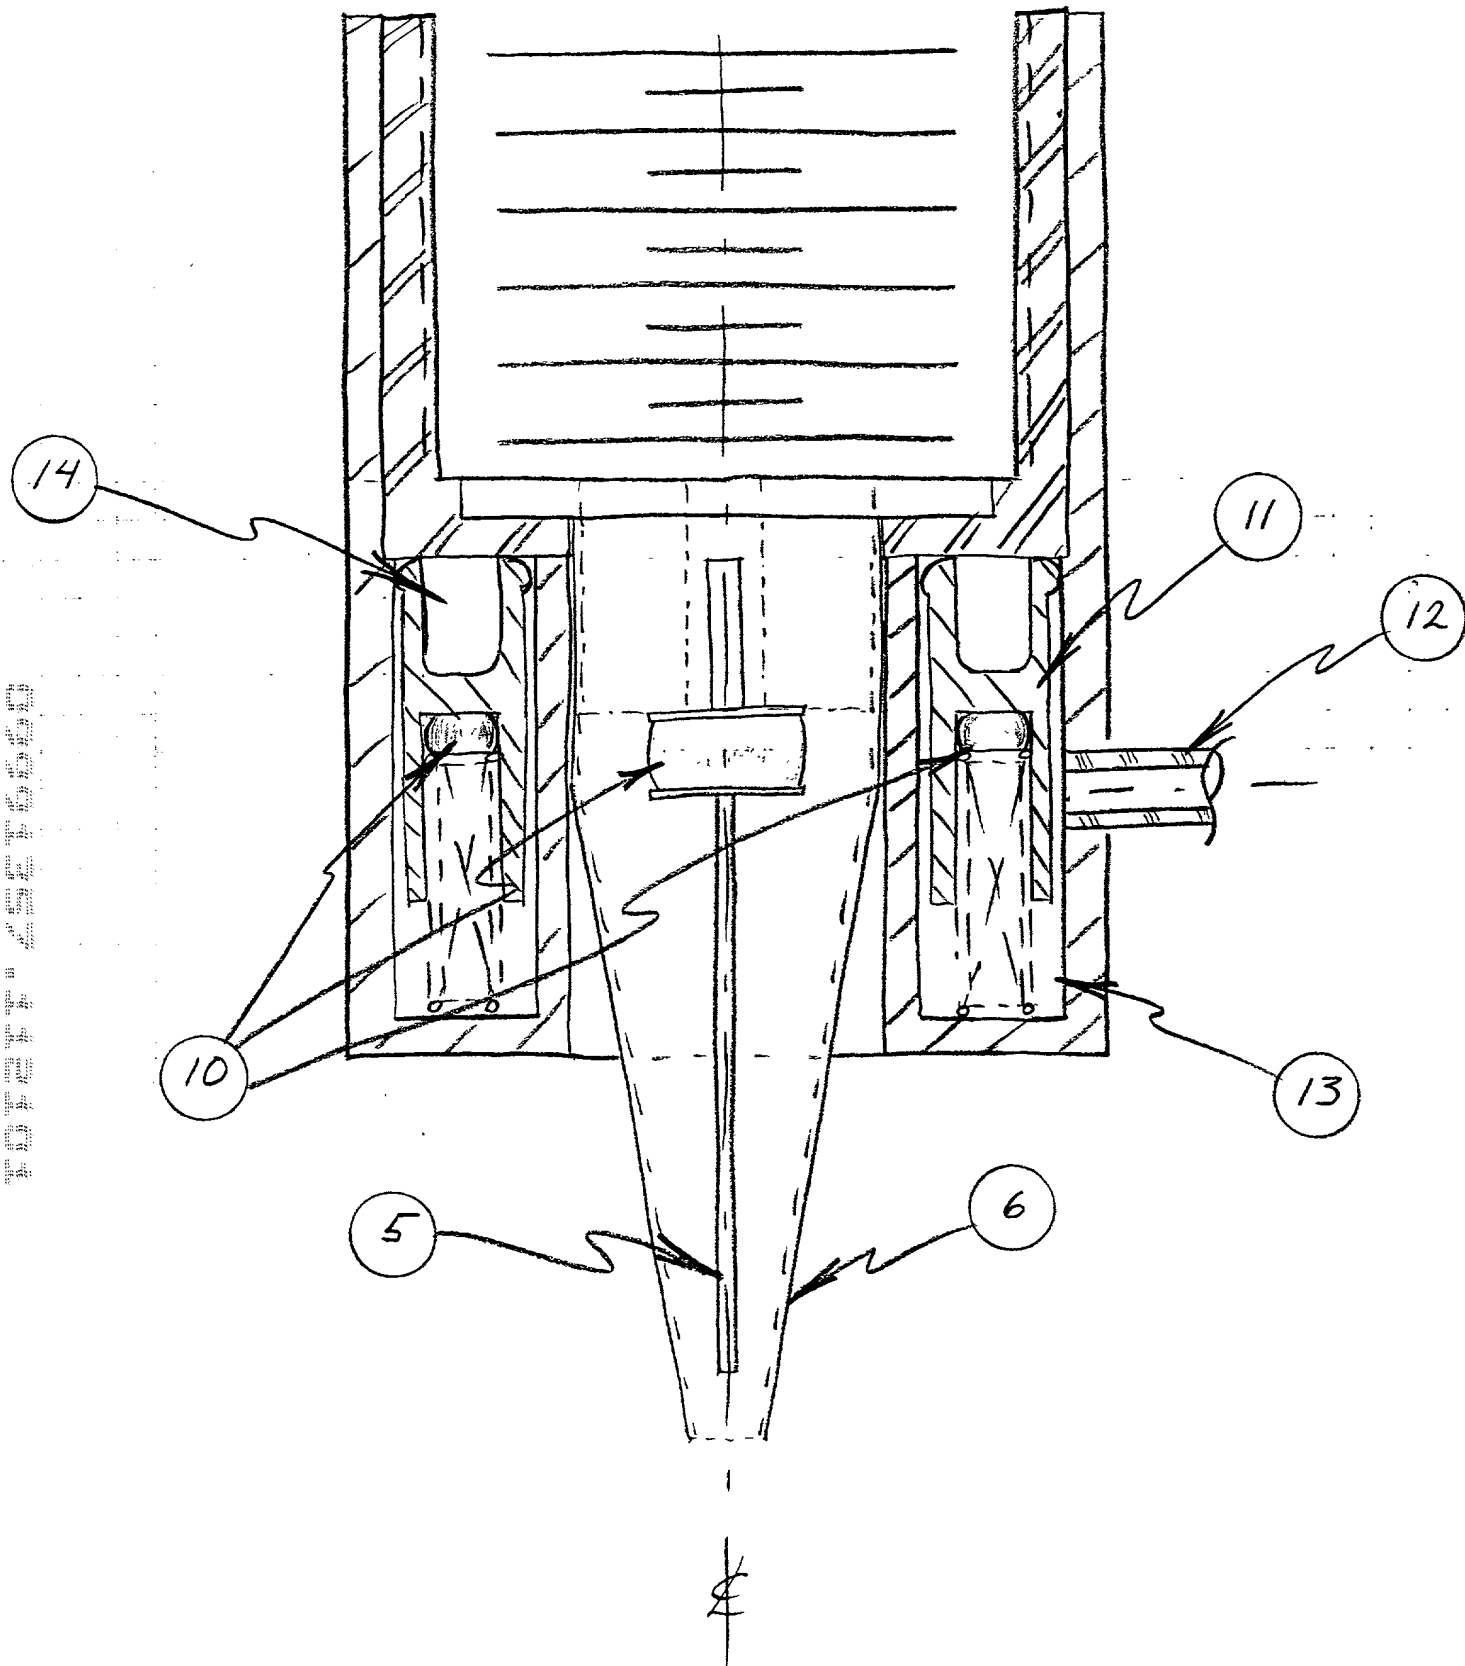


FIG. 2

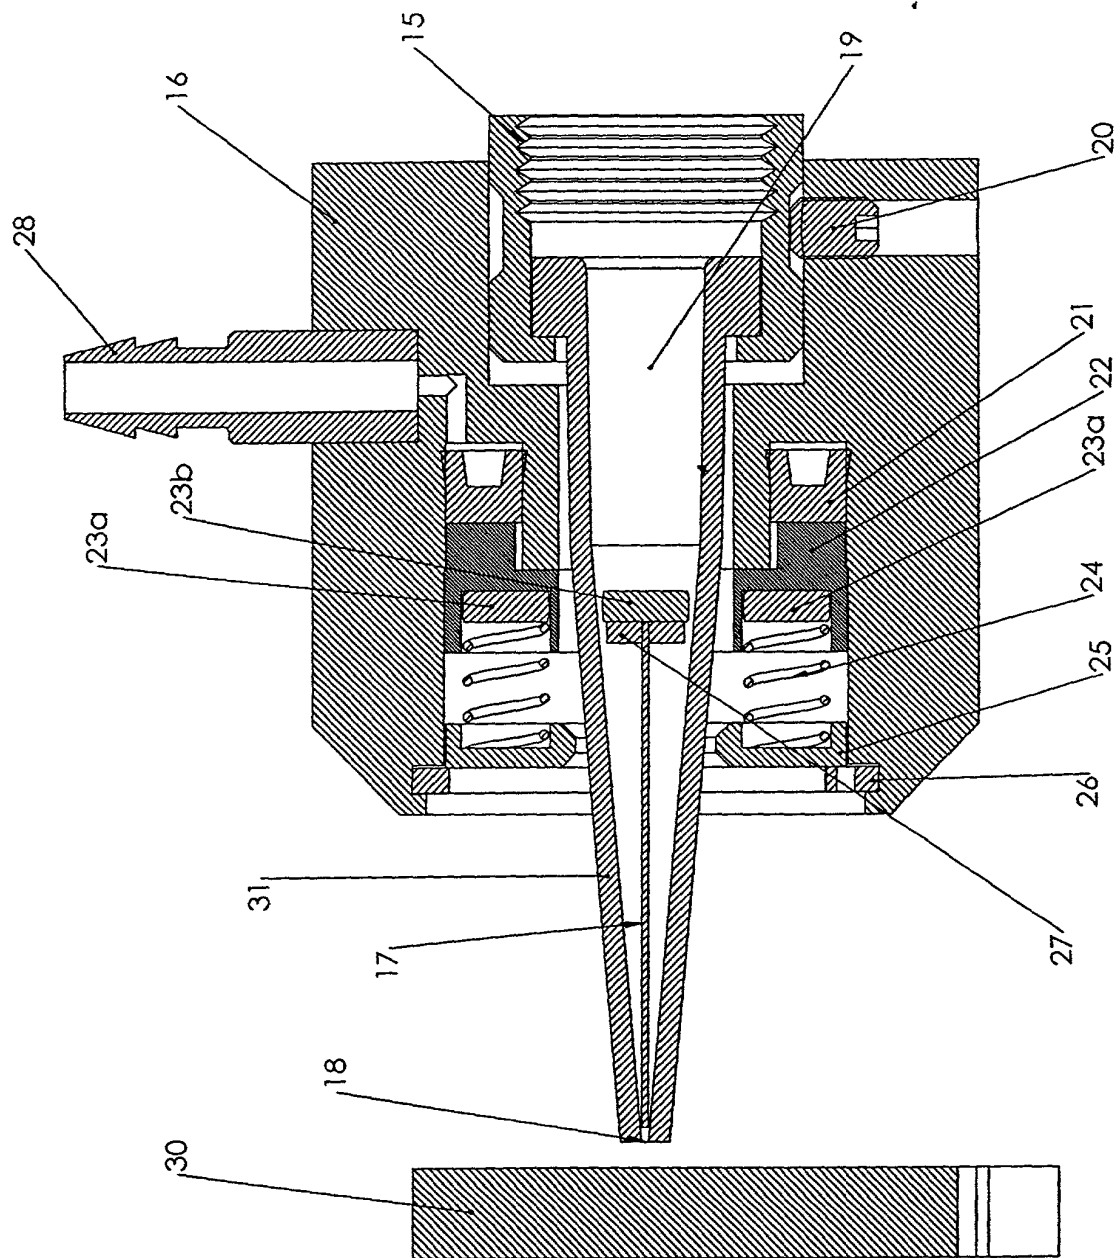


FIG. 3

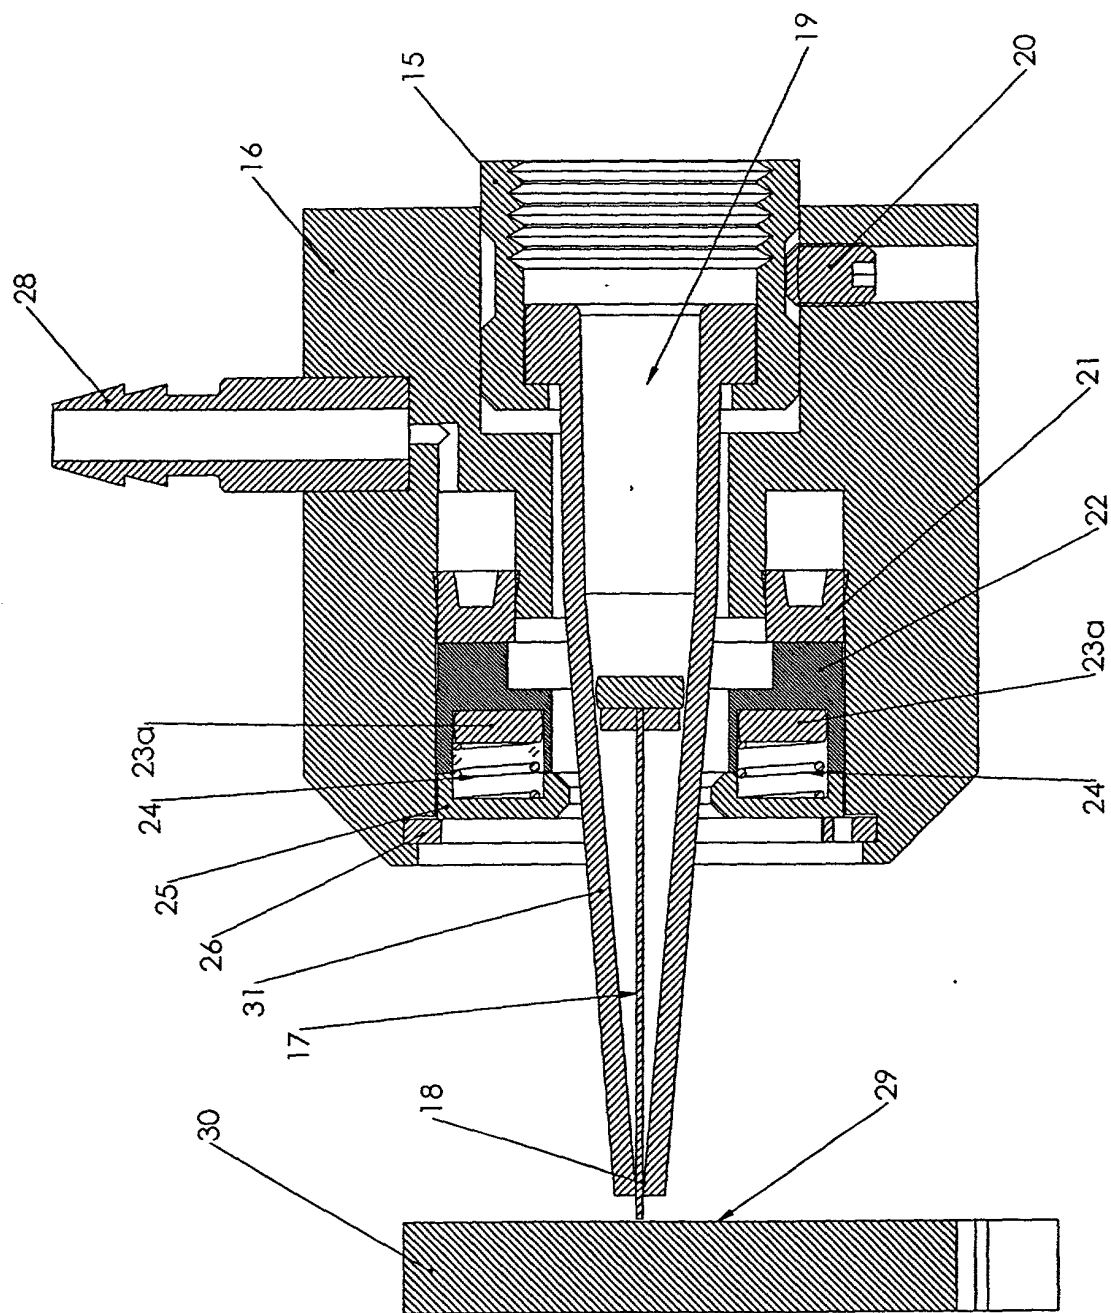


FIG. 4

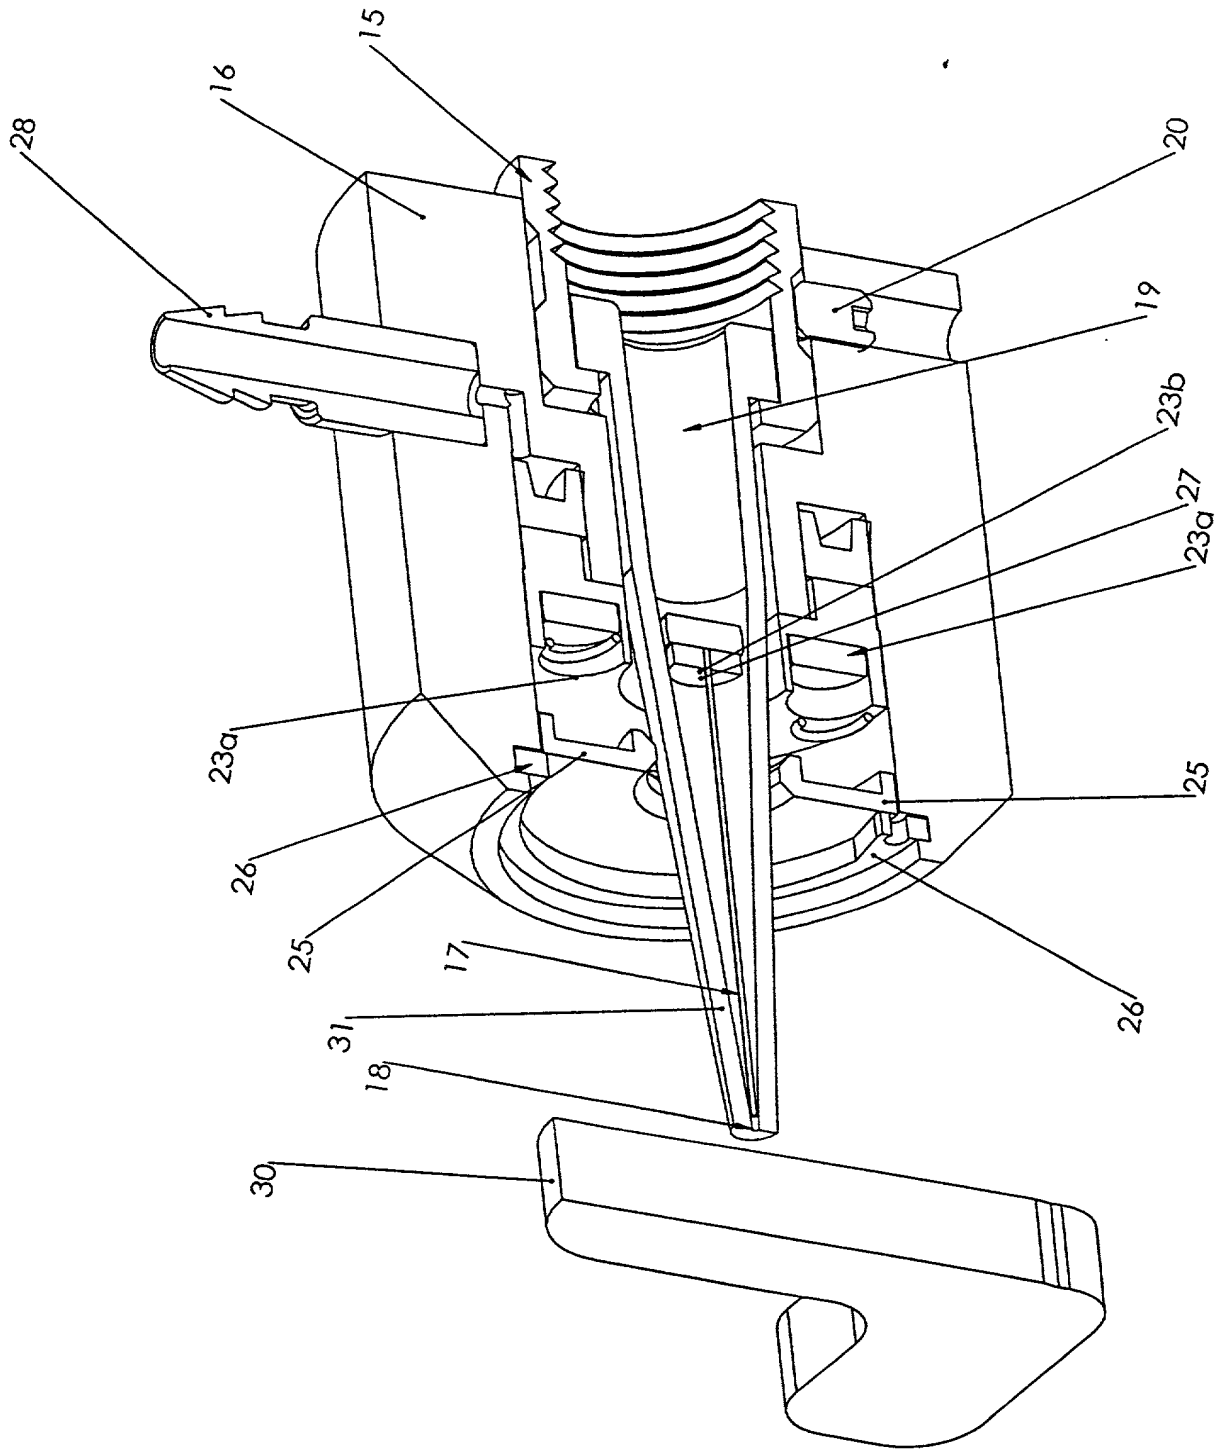


FIG. 5